

VERIFICATION OF CALIBRATION REPORT

of DataMaster dmt Breath Test Instrument

State of Alaska

Serial #: 100383

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Date: 05/25/2011

External Standard Test Values

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
TARGET AT 29.28: 0.078
LOT #: 02511080A2
EXPIRATION: 02/01/2013

BLANK TEST	0.000	08:59
INTERNAL STANDARD	VERIFIED	09:00
EXTERNAL STANDARD	0.081	09:00
BLANK TEST	0.000	09:01
EXTERNAL STANDARD	0.079	09:01
BLANK TEST	0.000	09:02
EXTERNAL STANDARD	0.079	09:02
BLANK TEST	0.000	09:03
EXTERNAL STANDARD	0.079	09:03
BLANK TEST	0.000	09:04
EXTERNAL STANDARD	0.079	09:05
BLANK TEST	0.000	09:05

Average = 0.0794
Std Dev = 0.0009

Diagnostic Check

VERSIONS
DMT: 1.02
PIC: 3.02
Modem: 2.0
Questions: 2.2

TEMPERATURES

Sample Chamber = 48.7°C	PASSED
Breath Tube = 47.8°C	PASSED

PUMP INFO

Flow Rate = 4.800 L/M	PASSED
-----------------------	--------

DETECTOR INFO

PUMP ON	PASSED
PUMP OFF	PASSED


FILTER INFO

Filter 1	PASSED
Filter 2	PASSED
Filter 3	PASSED



INTERNAL STANDARD	PASSED
-------------------	--------


I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the Breath Alcohol Program, which includes assuring that instruments are calibrated and maintaining program records.
- (5) The above is a true and accurate verification of calibration, which is performed by the instrument's software, as specified by the State Breath Alcohol Program. Verification of calibration is a regularly conducted and regularly recorded activity of the State Breath Alcohol Program.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

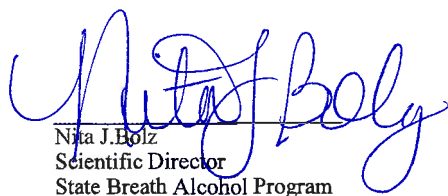 6/15/11
Nita J. Bolz
Scientific Director
State Breath Alcohol Program

Subscribed and sworn before me this 15 day of JUNE, 20 11

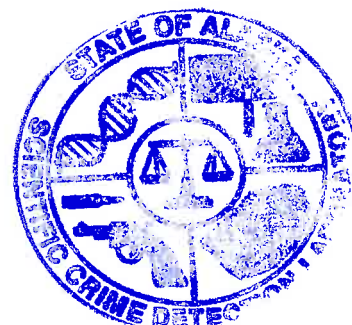


Notary Public's Signature
My Commission Expires on W 104 OFFICE
Notary Name
Kyle Klopfer

BMB
5/25/11